(19) Europäisches Patentamt
European Patent Office
Offic européen des brevets

(11) EP 1 132 136 A2

(12) EUROPEAN PATENT APPLICATION

(43) Date of publication:
12.09.2001 Bulletin 2001/37

(51) Int Cl.[7]: **B01L 3/02**, B01J 19/00, G01N 21/88

(21) Application number: **01104785.9**

(22) Date of filing: **27.02.2001**

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE TR
Designated Extension States:
AL LT LV MK RO SI

(30) Priority: **06.03.2000 JP 2000060787**

(71) Applicant: **Hitachi Software Engineering Co., Ltd.**
Yokohama-shi, Kanagawa 231-8475 (JP)

(72) Inventors:
- ***Yamamoto, Tomoyuki***
  Yokohama-shi, Kanagawa 231-8475 (JP)
- **Tamura, Takuro**
  Yokohama-shi, Kanagawa 231-8475 (JP)

(74) Representative: **Liesegang, Roland, Dr.-Ing.**
FORRESTER & BOEHMERT
Franz-Joseph-Strasse 38
80801 München (DE)

(54) Microarray, method for producing the same, and method for correcting inter-pin spotting amount error of the same

(57) The present invention has an objective of obtaining more accurate data of microarray experiments by correcting an inter-pin spotting amount error caused upon microarray production using a plurality of pins.

Upon microarray production, samples are immobilized on a microarray support using all pins as controls for correcting the inter-pin spotting amount errors. After the microarray experiments, luminescent intensities of the samples used as control spots for correcting the inter-pin spotting amount errors are measured and used to obtain correction parameters for the inter-pin spotting amount errors of respective pins. These parameters are used to correct luminescent intensities of other samples.

Fig. 2

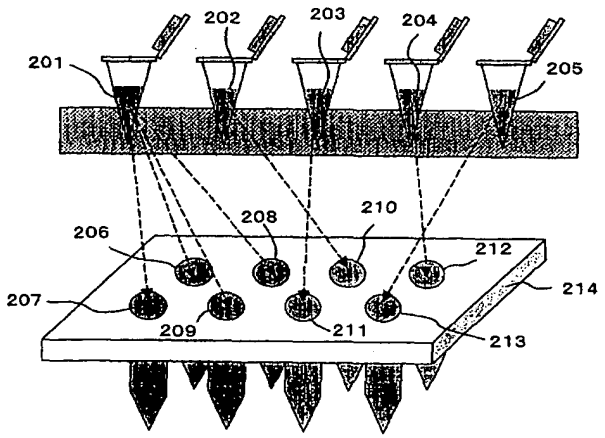

EP 1 132 136 A2

Printed by Jouve, 75001 PARIS (FR)

Description

FIELD OF THE INVENTION

[0001] The present invention relates to a microarray, a method for producing the same using pins, and a method for correcting inter-pin spotting amount errors of the same.

BACKGROUND OF THE INVENTION

[0002] In the fields of molecular biology and biochemistry, biopolymers such as nucleic acids and proteins from organisms are identified and/or fractionated in order to search for useful genes or to diagnose diseases. A hybridization reaction is frequently used as a pretreatment for such process, where a target molecule in a sample is hybridized with a nucleic acid or a protein having a known sequence. For this purpose, microarrays, or so-called biochips or DNA chips, are used on which probes such as DNAs, RNAs or proteins with known sequences are immobilized at predetermined positions.

[0003] On a microarray, a plurality of regions called features are defined on which different probes are immobilized. The microarray is placed into a reaction container together with sample DNA or the like to allow the fluorescence-labeled sample DNA to hybridize with the probes immobilized on the respective features of the microarray. Thereafter, the microarray is irradiated with excitation light to measure fluorescent intensity of each feature. Based on the measured fluorescent intensities, the binding levels between the respective probes and the sample DNA are obtained and converted into desired information.

[0004] Currently, there are roughly two methods for producing microarrays. One is a method in which oligonucleotides are synthesized on a microarray support, and the other is a method in which samples such as cDNAs are spotted on a microarray support. The latter microarray production method generally uses pins for capturing samples from wells of a well plate storing the samples and immobilizing the samples onto the microarray support. In order to improve speed of producing the microarray, a plurality of pins are used simultaneously. Since many microarray experiments require to measure quantitative differences between the spots, great care should be taken to produce uniform pins and to accurately attach pins to a device not to cause any spotting amount error between the plurality of simultaneously-used pins.

[0005] However, as the number of the simultaneously-used pins are increased in order to perform faster microarray production, it becomes more difficult to equalize the spotting amounts of the pins by production of uniform pins and by accurate attachment of the pins to the device (i.e., by hardware means).

[0006] In view of the above-described problems, the present invention has objectives of providing a microarray which does not have an influence on measurement results even when there is a difference of spotting amount between pins, a method for producing such microarray, and a method for correcting an inter-pin spotting amount error of a microarray.

SUMMARY OF THE INVENTION

[0007] The present invention realizes the above-mentioned objectives by software means. Specifically, a particular sample is spotted using all of the pins to generate control spots (inter-pin error correction control spots) as a part of samples to be immobilized upon microarray production. Luminescent intensities of the inter-pin error correction control spots are measured using a microarray reader, thereby obtaining spotting amount error information. Correction parameters for the inter-pin errors are obtained for respective pins based on the obtained spotting amount errors to correct luminescent intensities of spots on the same microarray measured with the microarray reader, thereby obtaining corrected values for the measured values of the respective spots.

[0008] In order to correct the luminescent intensity of each spot, it is necessary to specify which spot has been spotted with which pin. The present invention comprises a database for storing information as to which sample has been taken from which well (coordinate positions) of a well plate storing samples to be immobilized on respective spots upon microarray production, and a program for tracing which pin is actually used for spotting that sample.

[0009] A microarray according to the present invention comprises a support on which a plurality of sample spots are arranged in a two-dimensional array, wherein the plurality of sample spots comprise a group of sample spots of identical samples as control spots having a predetermined positional relationship which are used for correcting spotting amount errors among sample spots belonging to other groups of sample spots having the same relative positional relationships as that of the group of control spots.

[0010] The sample spots belonging to the groups of sample spots may not be provided on the microarray in an adjacent manner. When the sample spots are to be immobilized on the microarray at a pitch narrower than pin intervals of the pins of the spotting device, the control spots are provided at skipped positions on the microarray.

[0011] According to a method of the invention for producing a microarray having a support on which a plurality of

sample spots are arranged in a two-dimensional array, an operation is repeated in which a plurality of samples are simultaneously spotted on the support by using a spotting device provided with a plurality of pins, wherein the method comprise a step of simultaneously spotting the same samples on the support with all of the pins of the spotting device. The identical samples simultaneously spotted using all of the pins of the spotting device act as control spots for measuring inter-pin spotting amount errors caused by differences between individual pins of the spotting device.

[0012] According to a method of the invention for correcting an inter-pin spotting amount error of a microarray produced by repeating an operation of simultaneously spotting a plurality of samples on a support by using a spotting device provided with a plurality of pins, the method comprises the steps of: simultaneously spotting the same samples as controls on the support with all of the pins of the spotting device, where a plurality of samples are spotted on the support with the spotting device; measuring spotting amounts of the controls spotted with the respective pins of the spotting device to obtain correction parameters for inter-pin spotting amount errors; and correcting a measured value of each sample spot on the support by using the obtained correction parameters for the inter-pin spotting amount errors.

[0013] The spotting amounts of the controls using respective pins of a spotting device may be measured after a hybridization reaction with a sample or before the hybridization. When the spotting amounts of the controls are to be measured after the hybridization reaction, for example, luminescent intensities from fluorescence-labeled samples hybridized to the controls may be measured as the spotting amounts of the controls. On the other hand, when the spotting amounts of the controls are to be measured before the hybridization reaction, for example, a predetermined level of fluorescent substance may be contained in the controls so that luminescent intensities from the fluorescent substances can be measured as the spotting amounts of the controls.

[0014] According to a method for correcting an inter-pin spotting amount error of the microarray, information for identifying the pins used for immobilizing the samples to respective sample spot locations may be obtained via positional information of wells on a well plate, which store the samples to be transferred to a microplate with the pins.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] Figure **1** is a diagram showing an outline of a measurement using a microarray of the invention.

[0016] Figure **2** is a schematic view showing a process for dispensing samples into a well plate.

[0017] Figures **3A** and **3B** are schematic views illustrating a process of producing a microarray by using a spotting device having a plurality of pins.

[0018] Figure **4** is a schematic view of a microarray reader.

[0019] Figures **5A** and **5B** are tables showing an exemplary structure and exemplary data of a microarray information database.

[0020] Figure 6 is a flowchart showing an outline of an operation by a luminescent intensity correcting program.

[0021] Figures **7A** to **7B** are views showing exemplary screens for displaying corrected values of luminescent intensities.

DETAILED DESCRIPTION OF THE INVENTION

[0022] Hereinafter, embodiments of the present invention will be described with reference to the attached drawings. Herein, a spotting device having four pins is exemplified for convenience. However, it is obvious that the present invention is equivalently applicable to microarrray production using a spotting device having more than four pins.

[0023] Figure 1 is a diagram showing an outline of a measurement using a microarray of the invention. For experiments using the microarray, a microarray information database **104** stores sample data, microarray production data and microarray data obtained during the course of preparation of various samples **101**, microarray producing apparatus **102** and microarray reader **103**. The data in the database **104** is used for identifying the various samples, for storing information as to which sample has been taken from which position of a well plate storing the samples, and for tracing which pin is actually used for spotting that sample. Once an order 107 is given for calculating corrected values of luminescent intensities of respective spots, a luminescent intensity correcting program **105** starts to calculate the corrected value of the luminescent intensity of each spot based on the information acquired from the microarray information database **104**, and displays the results on a display device **106**. Details of the microarray information database **104**, the luminescent intensity correcting program **105** and display on the display device **106** will be described later.

[0024] Figure **2** is a schematic view showing a process for dispensing samples **201** to **205** prepared for a microarray experiment into a well plate **214**. The samples **201** to **205** are samples to be immobilized on a microarray and are stored in respective Eppendorf tubes. The sample **201** is prepared as a control for correcting inter-pin spotting amount errors. The samples **202** to **205** are Samples 1 to Sample 4 as subjects of a test using the microarray. The sample **201** as a control for correcting the inter-pin spotting amount errors is necessary for obtaining corrected luminescent intensities of respective spots and is prepared like other samples.

[0025] As represented by broken arrows in Figure 2, the samples **201**, **202**, **203**, **204** and **205** in the Eppendorf tubes

are dispensed into wells **206** to **209**, a well **210**, a well **211**, a well **212** and a well **213** of a well plate **214**, respectively. The sample **201** (as the control for correcting the inter-pin spotting amount errors) needs to be dispensed into wells which are at positions where all of the plurality of pins of the spotting device used for immobilization on the microarray are simultaneously accessible to the samples.

[0026] At this point, information of the samples **202** to **205**, information as to which sample has been dispensed into which well on the well plate **214** and the like can be obtained. The obtained information is stored in the microarray information database **104** as sample spot information.

[0027] Figures **3A** and **3B** are schematic views illustrating a process of immobilizing samples from the respective wells of the well plate onto the microarray by using the spotting device having four pins. The spotting device **301** has four pins that are capable of simultaneously capturing four kinds of samples from the well plates **302a, 302b**.... Accordingly, four spots can be spotted on the microarray support **303** at the same time by a single spotting operation. As shown in Figure **3A**, tips of the four pins of the spotting device **301** are immersed into wells of the well plate **302a** containing the samples. Then, as shown in Figure **3B**, the tips of the pins of the spotting device **301** capturing the samples make contact with the microarray **303** at designated coordinate positions, whereby the samples on the tips of the pins transfer to the microplate to be immobilized thereon and form sample spots.

[0028] At this point, information of the pins or the like used for microarray production is stored in the microarray information database **104** as microarray information. Herein, the alignment between the positions of the samples on the well plates **302a, 302b**... and the positions on the microarray **303** will not specifically be mentioned since the operations with the pins for immobilizing samples may vary depending on a microarray producing apparatus. However, the alignment here is made suitable.

[0029] Figure **4** is a schematic view showing a process of reading luminescent intensities of respective spots on a produced microarray **401** and a background luminescent intensity of the microarray **401** itself by using a microarray reader **402**.

[0030] First, a fluorescence-labeled sample is hybridized with samples immobilized on the microarray according to a known method. Thereafter, the microarray **401** is placed beneath the reader **402** to be irradiated with excitation light from a excitation light source **403**. Luminescence from fluorescencelabels are read with a two-dimensional optical sensor **404**. An optical filter **405** which does not allow passage of the excitation light from the lamp **403** but permits passage of the luminescence from the fluorescence labels is arranged on an optical path of the two-dimensional optical sensor **404**. Data of read luminescent intensities of spots and information of the background value between the spots are sent to a computer **407** via a controller **406**. Information of luminescent intensity of each spot obtained by reading the microarray information with the microarray reader **402** and information of the background value of the microarray is stored in the microarray information database **104** as sample spot information and microarray information, respectively.

[0031] Figures **5A** and **5B** are tables showing an exemplary structure of the microarray information database **104**. The table shown in Figure **5A** shows exemplary records of information relative to microarrays, and includes fields such as microarray IDs **501**, background values **502** of the microarrays, definitions **503** of the microarrays and types of pins **504** used for microarray production. The table shown in Figure **5B** shows exemplary records of information relative to spots immobilized on the microarray, and includes fields such as spot IDs **505**, pointers to the microarray information (microarray IDs) **506**, sample names **507**, definition information **508**, luminescent intensities **509** and positional information **600** and **601** of wells on the well plate.

[0032] Based on these data, a pin used for immobilizing a sample on each spot location is specified from a plurality of pins (herein, four pins) of a single spotting device **301** to obtain a correction parameter for an inter-pin spotting amount error for the pin. The obtained correction parameters for the inter-pin spotting amount errors are used to calculate a corrected value of the luminescent intensity of each spot, which will be described below.

[0033] Figure **6** is a flowchart showing an outline of an operation by the luminescent intensity correcting program 105 used for calculating a corrected value of the luminescent intensity of each spot. Once the program starts, first samples used as inter-pin spotting amount error correction controls are specified. Information of these samples such as luminescent intensities thereof, well coordinates information thereof and a type of pins used for immobilizing the samples onto the microarray is acquired from the microarray information database **104 (S601)**. In this example, it can be found from the sample spot information shown in Figure **5B**, that four spots designated spot IDs **SS1** to **SS4** are derived from the control samples, that the luminescent intensities of these control samples are 4500, 4600, 4400 and 4700, respectively, and that X-Y coordinates of wells containing the respective control samples are (1, 1), (1, 2), (2, 1) and (2, 2), respectively. Further information can be obtained from the microarray information shown in Figure 5A that the pin type of the microarray designated microarray ID **MA1** is 2 x 2 and that the background value is 100.

[0034] Next, from the coordinates information of the wells and pin type information, pins used for immobilizing the respective samples as the controls for correcting the inter-pin spotting amount errors are specified as a set of pin specifying variables (A, B) as calculated by the following [Equation 1] and [Equation 2] **(S602)**.

[Equation 1]

$$X = \frac{\text{X-coordinate of the well}}{\text{Number of pins along x-axis}}$$

$$Y = \frac{\text{Y-coordinate of the well}}{\text{Number of pins along y-axis}}$$

X': An integer of X, where the first place of decimal is counted as a whole number when not 0.
Y': An integer of Y, where the first place of decimal is counted as a whole number when not 0.

[Equation 2]

Pin specifying variable A = x-coordinate of the well -

(X' - 1) x number of pins along x-axis

Pin specifying variable B = y-coordinate of the well -

(Y' - 1) x number of pins along y-axis

[0035] The above-mentioned [Equation 1] and [Equation 2] are used for determining the pin specifying variables indicating one of the plurality of pins of the spotting device 301, which is used for immobilizing a particular sample onto the microarray. A group of wells storing samples that are captured with the plurality of pins at a time is considered as a single block. [Equation 1] determines a block that meets at the x- and y-coordinates, to which a particular well belong. [Equation 2] gives x-y coordinates of the particular well within the block to which it belongs by subtracting the blocks at the left of and above the block determined by [Equation 1]. Since a single block is a group of wells of samples that are captured with the pins at a time, the obtained coordinates correspond to x-y coordinates of the pin used for the particular well. By using the obtained x- and y-coordinates as pin specifying variables, the pin used for immobilizing the sample in the particular well on the microarray can be specified. In the case of arrangement shown in Figure 3, pin variables (A, B) determined by above [Equation 1] and [Equation 2] will result in four coordinate sets {(1, 1), (2, 1), (1, 2), (2, 2)}.

[0036] Next, correction parameters C.P.(A, B) for inter-pin spotting amount errors of the plurality of pins (A, B) of the spotting device **301** are determined. For this purpose, the above-mentioned pin specifying variables of the respective pins, luminescent intensities of samples used as inter-pin spotting amount error correction controls, and the background value BG of the microarray are used **(S603).**

[0037] A correction parameter C.P.(A, B) for inter-pin spotting amount error of a particular pin specified by pin specifying variables (A, B) is determined by the following [Equation 3].

[Equation 3]

$$C.P.(A, B) = \frac{\text{Average value of luminescent intensities of controls}}{\text{Luminescent intensity of control of pin (A, B) - BG}}$$

[0038] The average value of the luminescent intensities of the controls as the dividend of [Equation 3] is obtained by dividing the sum of the luminescent intensities of all controls by the number of the controls, and subtracting the background value BG of the microarray from the obtained value. Thus, correction parameters C.P.(1, 1), C.P.(2, 1), C.P.(1, 2) and C.P.(2, 2) are obtained for the inter-pin spotting amount errors of the four pins.

[0039] Then, a luminescent intensity of a particular sample whose corrected value is desired and coordinates information of its well on the well plate are obtained from the microarray information database 104**(S604)**.

[0040] Based on the coordinates information of the well of the particular sample and pin type information, pin specifying variables (A, B) are determined by above [Equation 1] and [Equation 2] for the pin used for spotting that particular sample. Sample spots having identical pin specifying values are samples spotted with the same pin. Thus, the pin used for spotting the particular sample on the microarray can be specified **(S605)**.

[0041] By using the inter-pin spotting amount error correction parameter C.P (A, B) of the pin used for immobilizing the sample, the corrected luminescent intensity (corrected value) is calculated by the following [Equation 4] (S606).

[Equation 4]

Corrected value =

C.P. (A, B) x (luminescent intensity of the sample - BG)

[0042] When corrected intensity values of more than one sample need to be calculated, Steps **604** to **607** are repeated until calculation of the corrected values for all of the desired samples are judged to be completed at Step **607**. Finally, the determined corrected values of the luminescent intensities of respective samples are displayed on a screen **(S608)**.

[0043] Figures **7A** to **7C** are views showing exemplary screens. As shown in Figure **7A**, a screen **701** for displaying corrected luminescent intensities includes information such as sample names, pins used for immobilizing the respective samples, measured luminescent intensities and corrected luminescent intensities of the respective samples, and correction parameters for inter-pin spotting amount errors for the respective pins. As shown in Figure **7B**, a command "selective display" or "sort" can be selected from [Edit] menu on a menu bar **702** of the corrected value displaying screen **701** to open a dialog box **703** for selective display or a dialog box **704** for sorting as shown in Figure 7C. By operation on these dialog boxes, data displayed on the corrected value displaying screen **701** can be processed.

[0044] According to the above description, correction parameters C.P. (A, B) for inter-pin spotting amount errors of a microarray are determined after a hybridization reaction of the microarray. However, correction parameters C.P.(A, B) for inter-pin spotting amount errors of a microarray may be determined by measuring control spots already containing a fluorescent substance after sample spotting and before a hybridization reaction.

[0045] According to the present invention, luminescent intensity errors caused by spotting amount errors between individual pins upon microarray production can be corrected, thereby obtaining measurement results that are not influenced by the quality of the hardware.

Claims

1. A microarray comprising a support (214;302 a,b,c) on which a plurality of sample spots (206 to 213) is arranged in a two-dimensional array,

   wherein the plurality of sample spots (206 to 213) comprise a group of sample spots (206 to 209) of identical samples as control spots having a predetermined positional relationship which are used for correcting spotting amount errors among sample spots (210 to 213) belonging to other groups of sample spots having the same relative positional relationships as that of the group of control spots.

2. A microarray according to claim 1, wherein the sample spots belonging to the group of sample spots are not provided on the microarray in an adjacent manner.

3. A method for producing a microarray having a support(214; 302 a, b, c) on which a plurality of sample spots (206 to 213) are arranged in a two-dimensional array, by repeating an operation of simultaneously spotting a plurality of samples on the support by using a spotting device provided (301) provided with a plurality of pins, wherein the method comprise a step of simultaneously spotting the same samples on the support with all of the pins of the spotting device.

4. A method for correcting an inter-pin spotting amount error of a microarray produced by repeating an operation of simultaneously spotting a plurality of samples (206 to 213) on a support (302 a, b, c) by using a spotting device (301) provided with a plurality of pins, the method comprising the steps of:

   simultaneously spotting the same samples as controls on the support with all of the pins of the spotting device, where a plurality of samples are spotted on the support with the spotting device;
   measuring spotting amounts of the controls spotted with the respective pins of the spotting device to obtain correction parameters for inter-pin spotting amount errors; and
   correcting a measured value of each sample spot on the support by using the obtained correction parameters for the inter-pin spotting amount errors.

5. A method for correcting an inter-pin spotting amount error of a microarray according to claim 4, wherein information for identifying the pins used for immobilizing the samples to respective sample spot locations is obtained via positional information of wells on a well plate, which store the samples to be transferred to a microplate with the pins.

Fig. 1

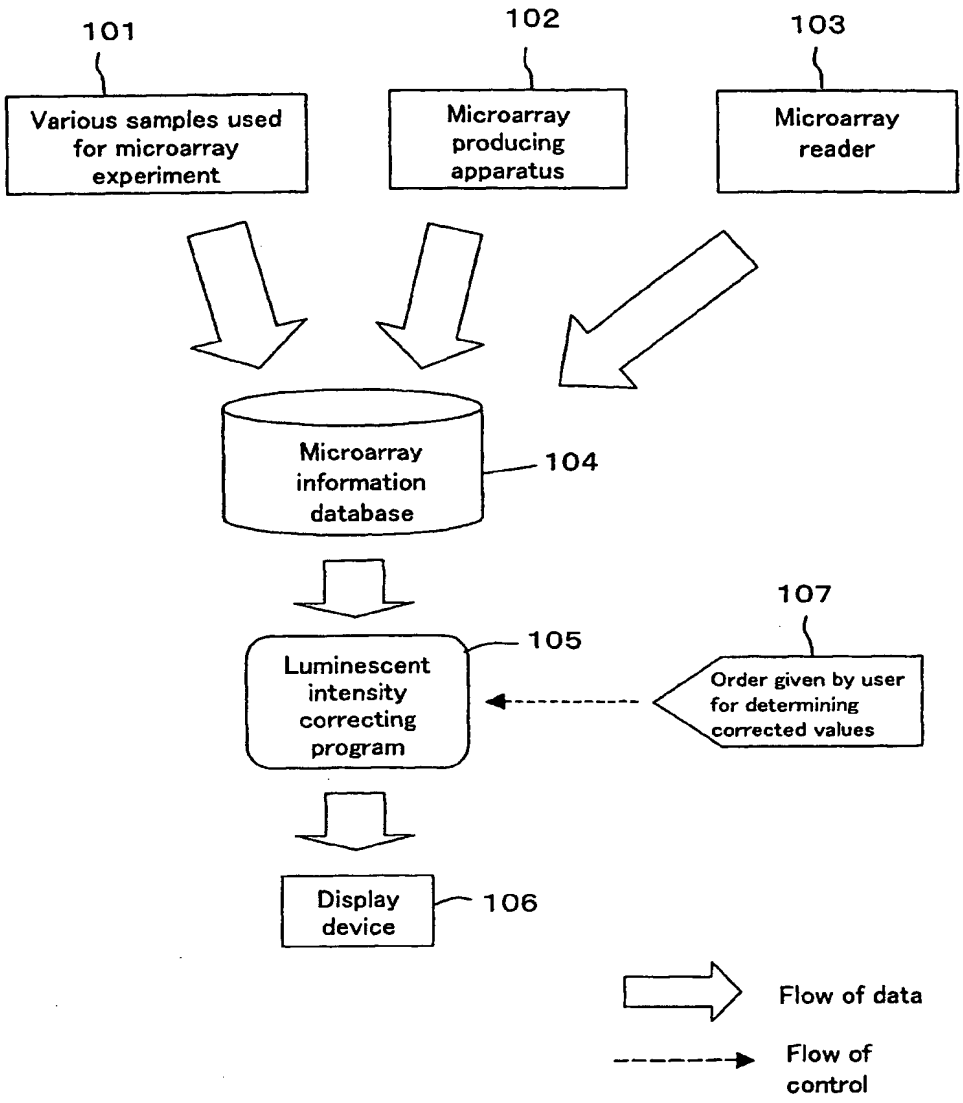
101
Various samples used for microarray experiment
102
Microarray producing apparatus
103
Microarray reader
Microarray information database
104
107
105
Luminescent intensity correcting program
Order given by user for determining corrected values
Display device
106
Flow of data
Flow of control

Fig. 2

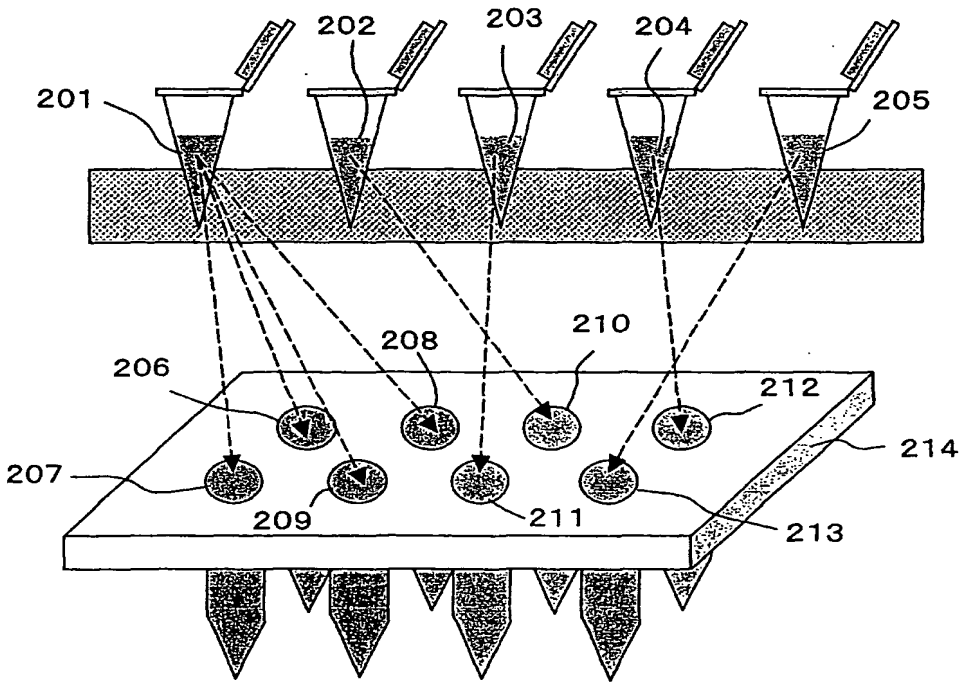

Fig. 3A

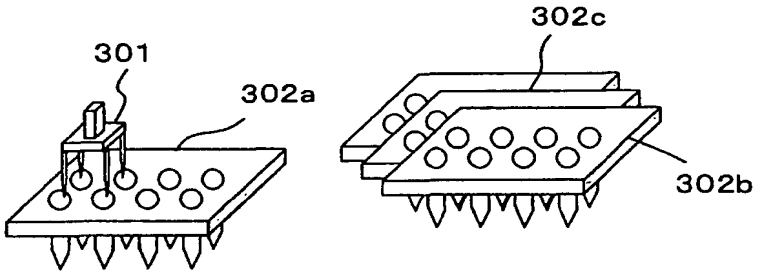

Fig. 3B

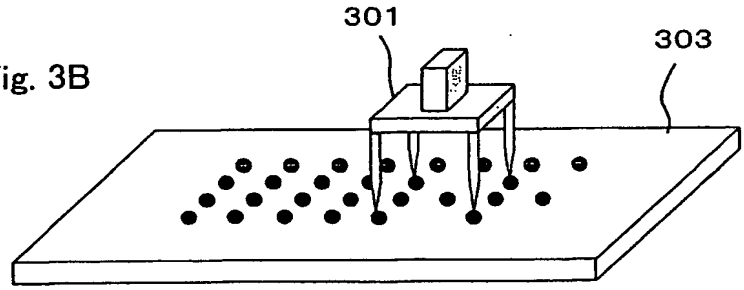

Fig. 4

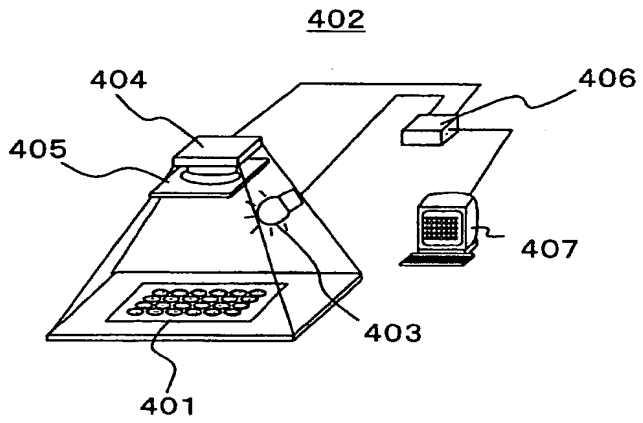

Fig. 5A

Microarray information

501 502 503 504

ID	Background value	Definition	Pin Type
MA1	100	Sample group from mouse tumor cell	2x2
MA2	....	....	...

Fig. 5B

Sample spot information

505 506 507 508 509 600 601

ID	MA ID	Sample Name	Definition	Luminescent intensity	X-coordinate of well	Y-coordinate of well
SS 1	MA1	Standard Control	Inter-pin spotting amount error correction control	4500	1	1
SS 2	MA1	Standard Control	Inter-pin spotting amount error correction control	4600	1	2
SS 3	MA1	Standard Control	Inter-pin spotting amount error correction control	4400	2	1
SS 4	MA1	Standard Control	Inter-pin spotting amount error correction control	4700	2	2
SS 5	MA1	Sample1	Sample 1 from mouse tumor cell	3000	3	1
SS 6	MA1	Sample2	Sample 2 from mouse tumor cell	4600	3	2
SS 7	MA1	Sample3	Sample 3 from mouse tumor cell	6500	4	1
SS 8	MA1	Sample4	Sample 4 from mouse tumor cell	1000	4	2

Fig. 6

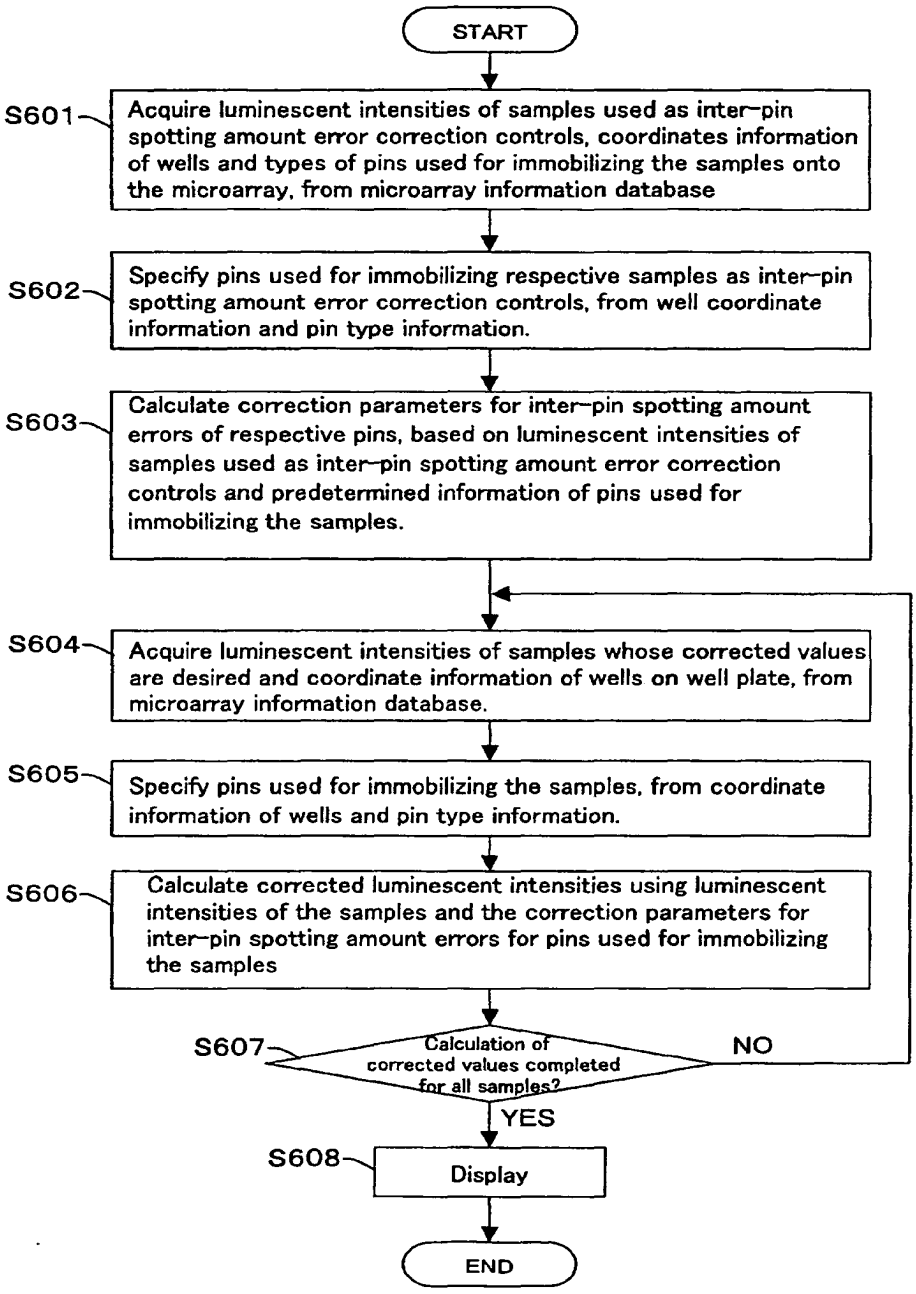
START
S601
Acquire luminescent intensities of samples used as inter-pin spotting amount error correction controls, coordinates information of wells and types of pins used for immobilizing the samples onto the microarray, from microarray information database
S602
Specify pins used for immobilizing respective samples as inter-pin spotting amount error correction controls, from well coordinate information and pin type information.
S603
Calculate correction parameters for inter-pin spotting amount errors of respective pins, based on luminescent intensities of samples used as inter-pin spotting amount error correction controls and predetermined information of pins used for immobilizing the samples.
S604
Acquire luminescent intensities of samples whose corrected values are desired and coordinate information of wells on well plate, from microarray information database.
S605
Specify pins used for immobilizing the samples, from coordinate information of wells and pin type information.
S606
Calculate corrected luminescent intensities using luminescent intensities of the samples and the correction parameters for inter-pin spotting amount errors for pins used for immobilizing the samples
S607
Calculation of corrected values completed for all samples?
NO
YES
S608
Display
END

Fig. 7A

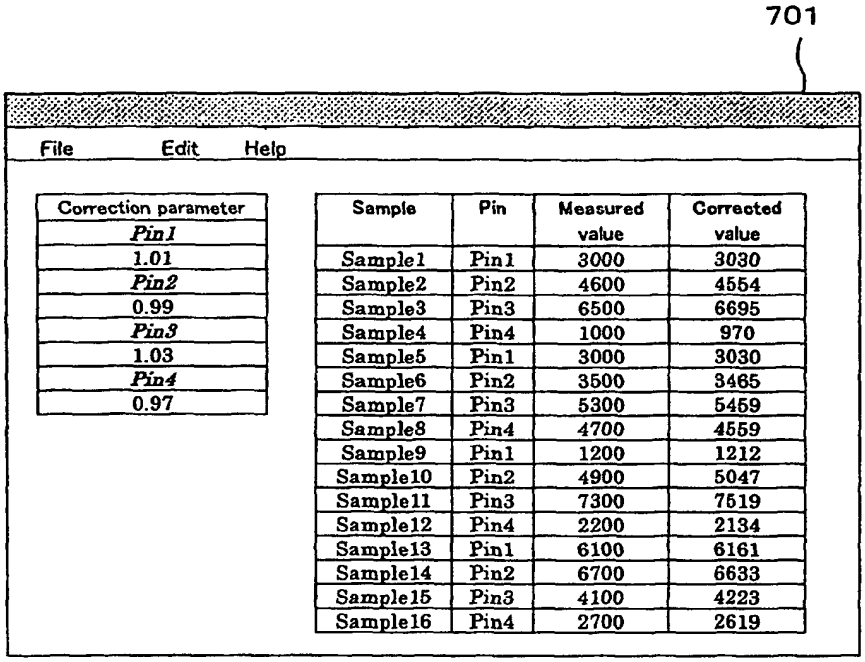

Correction parameter
Pin1
1.01
Pin2
0.99
Pin3
1.03
Pin4
0.97

Sample	Pin	Measured value	Corrected value
Sample1	Pin1	3000	3030
Sample2	Pin2	4600	4554
Sample3	Pin3	6500	6695
Sample4	Pin4	1000	970
Sample5	Pin1	3000	3030
Sample6	Pin2	3500	3465
Sample7	Pin3	5300	5459
Sample8	Pin4	4700	4559
Sample9	Pin1	1200	1212
Sample10	Pin2	4900	5047
Sample11	Pin3	7300	7519
Sample12	Pin4	2200	2134
Sample13	Pin1	6100	6161
Sample14	Pin2	6700	6633
Sample15	Pin3	4100	4223
Sample16	Pin4	2700	2619

Fig. 7B

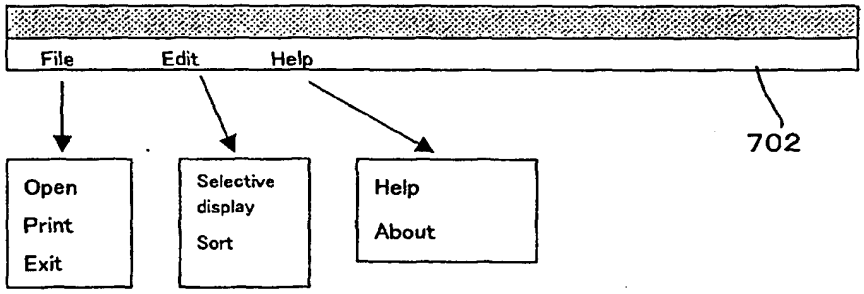

Fig. 7C

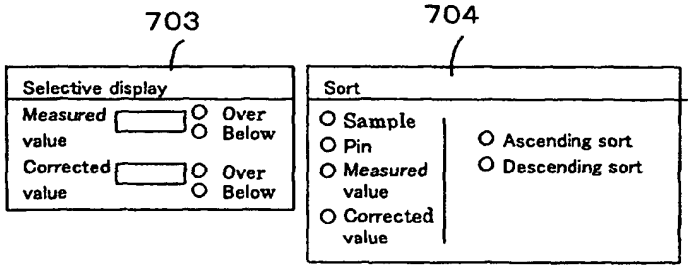

(19) Europäisches Patentamt
European Patent Office
Office européen des brevets

(11) EP 1 132 136 A3

(12) EUROPEAN PATENT APPLICATION

(88) Date of publication A3:
02.07.2003 Bulletin 2003/27

(43) Date of publication A2:
12.09.2001 Bulletin 2001/37

(21) Application number: **01104785.9**

(22) Date of filing: **27.02.2001**

(51) Int Cl.7: **B01L 3/02**, B01J 19/00, G01N 21/88, G01N 35/10

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE TR
Designated Extension States:
AL LT LV MK RO SI

(30) Priority: **06.03.2000 JP 2000060787**

(71) Applicant: **Hitachi Software Engineering Co., Ltd.**
Yokohama-shi, Kanagawa 231-8475 (JP)

(72) Inventors:
- **Yamamoto, Tomoyuki**
  Yokohama-shi, Kanagawa 231-8475 (JP)
- **Tamura, Takuro**
  Yokohama-shi, Kanagawa 231-8475 (JP)

(74) Representative: **Liesegang, Roland, Dr.-Ing.**
FORRESTER & BOEHMERT
Pettenkoferstrasse 20-22
80336 München (DE)

(54) Microarray, method for producing the same, and method for correcting inter-pin spotting amount error of the same

(57) The present invention has an objective of obtaining more accurate data of microarray experiments by correcting an inter-pin spotting amount error caused upon microarray production using a plurality of pins.

Upon microarray production, samples are immobilized on a microarray support using all pins as controls for correcting the inter-pin spotting amount errors. After the microarray experiments, luminescent intensities of the samples used as control spots for correcting the inter-pin spotting amount errors are measured and used to obtain correction parameters for the inter-pin spotting amount errors of respective pins. These parameters are used to correct luminescent intensities of other samples.

Fig. 2

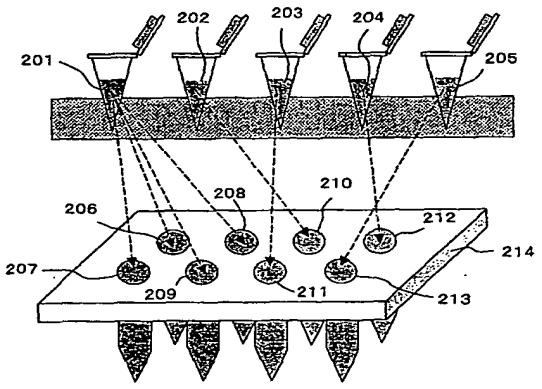

EP 1 132 136 A3

European Patent Office

EUROPEAN SEARCH REPORT

Application Number
EP 01 10 4785

DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
A	WO 99 22867 A (PERKIN ELMER CORP) 14 May 1999 (1999-05-14) * page 1, line 29 - page 3, line 2 * ---	1	B01L3/02 B01J19/00 G01N21/88 G01N35/10
A	SCHENA M ET AL: "Microarrays: biotechnology's discovery platform for functional genomics" TRENDS IN BIOTECHNOLOGY, ELSEVIER PUBLICATIONS, CAMBRIDGE, GB, vol. 16, no. 7, 1 July 1998 (1998-07-01), pages 301-306, XP004145643 ISSN: 0167-7799 * page 303; figure 2 * ---	1	
A	ROSE S D: "APPLICATION OF A NOVEL MICROARRAYING SYSTEM IN GENOMICS RESEARCH AND DRUG DISCOVERY" JOURNAL OF THE ASSOCIATION FOR LABORATORY AUTOMATION, XX, XX, vol. 3, no. 3, July 1998 (1998-07), pages 53-56, XP000957979 * page 56 * -----	1	TECHNICAL FIELDS SEARCHED (Int.Cl.7) B01L B01J G01N

The present search report has been drawn up for all claims

Place of search	Date of completion of the search	Examiner
MUNICH	9 May 2003	Tragoustis, M

CATEGORY OF CITED DOCUMENTS

X : particularly relevant if taken alone
Y : particularly relevant if combined with another document of the same category
A : technological background
O : non-written disclosure
P : intermediate document

T : theory or principle underlying the invention
E : earlier patent document, but published on, or after the filing date
D : document cited in the application
L : document cited for other reasons

& : member of the same patent family, corresponding document

EPO FORM 1503 03.82 (P04C01)

ANNEX TO THE EUROPEAN SEARCH REPORT ON EUROPEAN PATENT APPLICATION NO. EP 01 10 4785

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

09-05-2003

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9922867 A	14-05-1999	AT 215401 T	15-04-2002
		AU 748226 B2	30-05-2002
		AU 1292099 A	24-05-1999
		CA 2307141 A1	14-05-1999
		DE 69804653 D1	08-05-2002
		DE 69804653 T2	28-11-2002
		EP 1027159 A1	16-08-2000
		JP 2001522033 T	13-11-2001
		WO 9922867 A1	14-05-1999
		US 6228659 B1	08-05-2001

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82